


## Nitrile Examination Gloves

**Glove Plus Prime Nitrile** examination gloves offer high quality, cost effective, barrier protection against biohazards and a wide range of general chemicals glove users come into contact with on a regular basis.

Manufactured in a dedicated Nitrile factory, this product is 100% Natural Rubber Latex free and is ideal for glove users who have been identified as having allergic reactions to NR Latex proteins (Type 1 reactions).

### Product Key Points

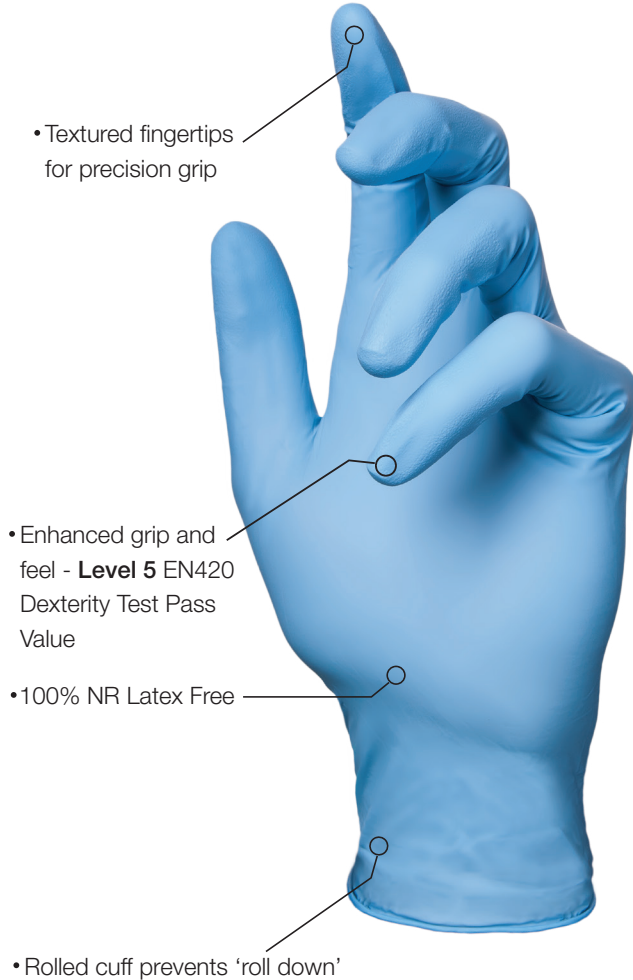

### Product Conformance:

- EU MDD EN455 Parts 1 & 2 - Medical Grade.
- Independently test by an EU Notified Body as meeting the requirements of EU PPE 89/686/EEC (Class III) "Protection Against Chemical Hazard"
- EN374 Parts 1, 2 & 3.
- EN420 Part 3.
- Passed an independent test to ISO 16604b:2004 "Resistance of Materials used in Protective Clothing to Penetration by Blood-Borne Pathogens" (viral test).
- EN420 Dexterity Test - Passed to the maximum Level 5.

### Product Information

- Type:** Powder free & non-sterile.
- Material:** Nitrile (Synthetic Latex) - Carbocylated Acrylonitrile Butadiene.
- Protein Content:** 100% NR Latex free.
- Powder Content:** Below 2mg/g glove.
- Features:** Ambidextrous, Beaded Cuff, Textured fingers.
- Colour:** Black, Blue & Pink.
- Packing:** 100 gloves per dispenser, 10 dispensers per carton.

### Dimensions

Glove Size	Product Colour			Palm Width (mm)	Length (mm)
	Blue	Black	Pink		
Extra Small	PN301	PNB301	PNP301	< 80	> 240mm
Small	PN302	PNB302	PNP302	± 80	> 240mm
Medium	PN303	PNB303	PNP303	± 95	> 240mm
Large	PN304	PNB304	PNP304	± 110	> 240mm
Extra Large	PN305	PNB305	PNP305	> 110	> 240mm

### Thickness

Location of Thickness Measurements		Single Wall (mm)
Finger	(at the tip)	0.085 ± 0.03
Palm	(at centre of palm)	0.065 ± 0.03

### Physical Properties

Parameters	Before Aging	After Aging
Force at Break (N)	>6.0	6.0
Watertight AQL	0.65	N/A

### Pre-Shipment Quality Inspection

Criteria	Insp Level	AQL
Dimensions	S-2	4.0
Physical Properties	S-2	4.0
1000ml Water Leak Test	G-1	1.5
Visual Inspection	S-4	4.0

### Quality Assurance:

- This product is manufactured in a plant where the quality management system has been independently assessed as conforming to ISO9001:2008 and ISO13485:2003.



www.glove-plus.com